

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 010 503 B

Burettes, 50 ml, str. stopc., amber grad., AS, conf. cert.




Batch: 27-23

Serial:

Measuring Nr. 73487

Batch size: 99

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	$\pm 0,0500$ ml	$\pm 0,0500$ ml	$\pm 0,0500$ ml
Average value:	50,0117 ml	30,0023 ml	10,0143 ml
Deviation:	0,0127 ml	0,0121 ml	0,0079 ml
Precision (CV):	0,0255 %	0,0402 %	0,0788 %

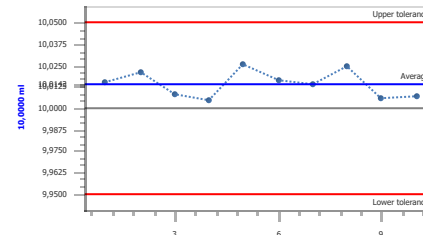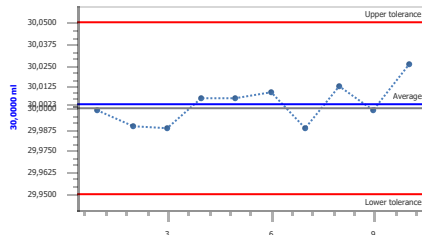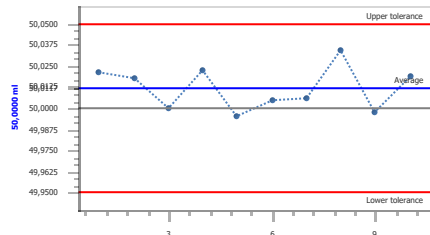

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

03.07.2025

Balance:

Sartorius -
LE244S-OCE

DE-M