

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 105

Burette, 10 ml, Schellb., lat. Valve, AS, conf. cert.

Batch: 31-22




Serial:

Measuring Nr. 72333

Batch size:

2

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	$\pm 0,0200$ ml	$\pm 0,0200$ ml	$\pm 0,0200$ ml
Average value:	9,9999 ml	5,9983 ml	2,0074 ml
Deviation:	0,0057 ml	0,0006 ml	0,0043 ml
Precision (CV):	0,0575 %	0,0095 %	0,2164 %

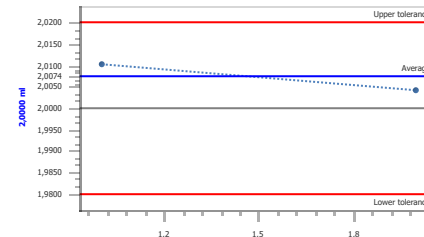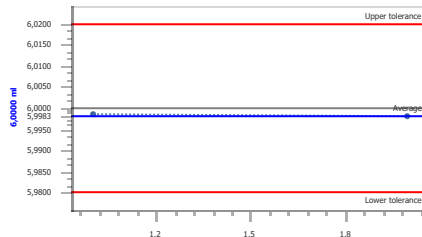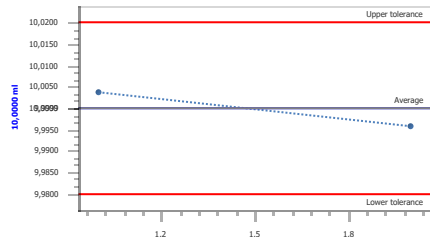

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

18.03.2025

Balance:

Sartorius -
LE244S-OCE

DE-M