

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 255

Burettes, 25 ml, lat. needle valve, AS, conf. cert.




Batch: 11-23

Serial:

Measuring Nr. 72995

Batch size: 20

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	$\pm 0,0300$ ml	$\pm 0,0300$ ml	$\pm 0,0300$ ml
Average value:	25,0098 ml	15,0048 ml	5,0030 ml
Deviation:	0,0055 ml	0,0089 ml	0,0074 ml
Precision (CV):	0,0221 %	0,0592 %	0,1483 %

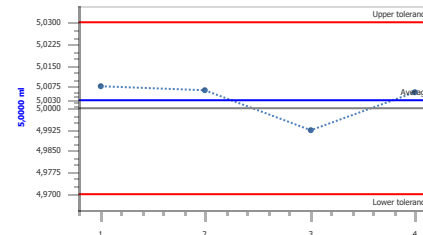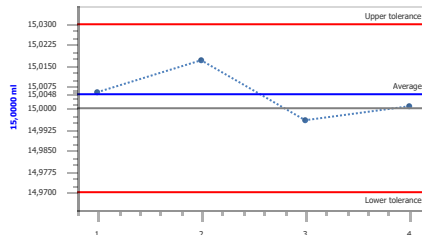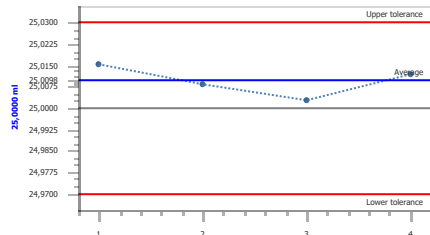

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

19.05.2025

Balance:

Sartorius -
LE244S-OCE

DE-M