

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 505

Burettes, 50 ml, lat. valve., Schellb., AS, conf. cert.




Batch: 13-25

Serial:

Measuring Nr. 72903

Batch size: 20

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	$\pm 0,0500$ ml	$\pm 0,0500$ ml	$\pm 0,0500$ ml
Average value:	50,0157 ml	30,0193 ml	10,0199 ml
Deviation:	0,0096 ml	0,0076 ml	0,0096 ml
Precision (CV):	0,0191 %	0,0254 %	0,0955 %

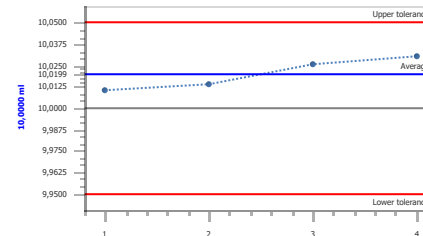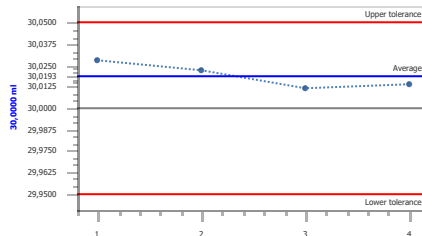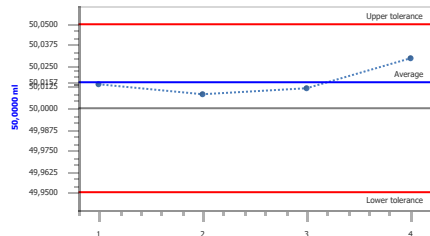

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

08.05.2025

Balance:

Sartorius - LC
6200 S

DE-M