

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 255

Pellet-burettes, 25 ml, lat. needle valve, AS, conf. cert.




Batch: 11-24

Serial:

Measuring Nr. 72217

Batch size: 20

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	$\pm 0,0300 \text{ ml}$	$\pm 0,0300 \text{ ml}$	$\pm 0,0300 \text{ ml}$
Average value:	25,0065 ml	15,0055 ml	5,0112 ml
Deviation:	0,0021 ml	0,0055 ml	0,0016 ml
Precision (CV):	0,0084 %	0,0365 %	0,0310 %

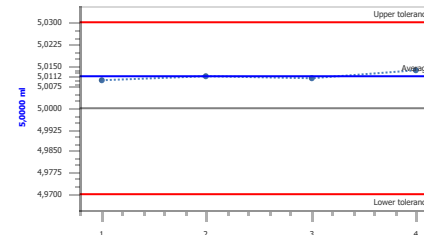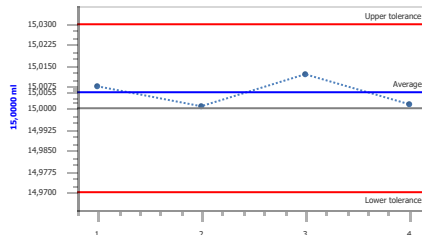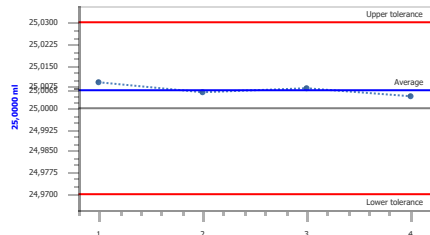

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

06.03.2025

Balance:

Sartorius -
LE244S-OCE

DE-M