

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 124 508

Pellet-burettes, 50 ml, amber glass, AS, conf. cert.

Batch: 18-22




Serial:

Measuring Nr. 78958

Batch size:

5

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	$\pm 0,0500$ ml	$\pm 0,0500$ ml	$\pm 0,0500$ ml
Average value:	50,0221 ml	30,0208 ml	10,0032 ml
Deviation:	0,0030 ml	0,0105 ml	0,0029 ml
Precision (CV):	0,0060 %	0,0351 %	0,0290 %

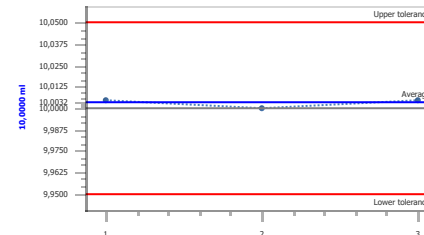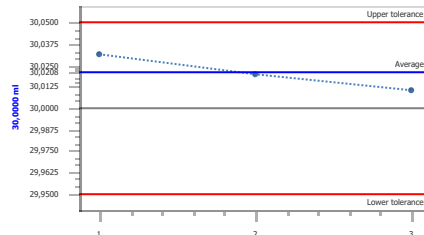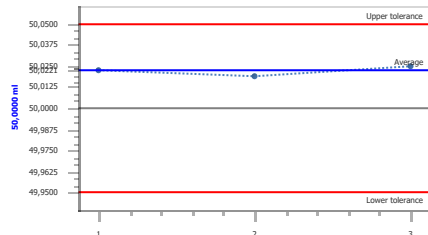

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

08.07.2026

Balance:

Sartorius -
LE244S-OCE

DE-M