

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 152 505

Univ. autom. burette, 50 ml, lat. valve, AS, conf. cert.

Batch: 45-21




Serial:

Measuring Nr. 73489

Batch size:

6

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	$\pm 0,0500$ ml	$\pm 0,0500$ ml	$\pm 0,0500$ ml
Average value:	50,0162 ml	30,0155 ml	10,0164 ml
Deviation:	0,0091 ml	0,0016 ml	0,0129 ml
Precision (CV):	0,0181 %	0,0052 %	0,1292 %

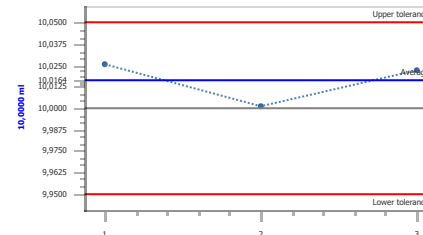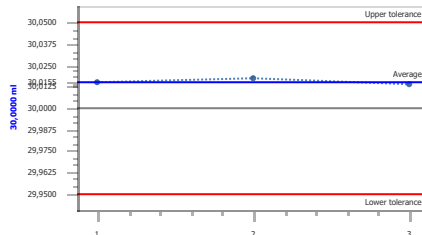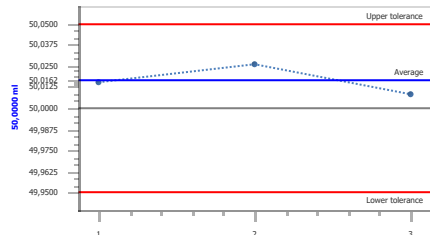

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

02.07.2025

Balance:

Sartorius -
LE244S-OCE

DE-M