

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 372 023

Micro burette, 2 ml, str. stopc., PTFE, AS, conf. cert.

Batch: 40-25




Serial:

Measuring Nr. 78957

Batch size:

6

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	$\pm 0,0100$ ml	$\pm 0,0100$ ml	$\pm 0,0100$ ml
Average value:	1,9991 ml	1,1964 ml	0,3972 ml
Deviation:	0,0021 ml	0,0021 ml	0,0022 ml
Precision (CV):	0,1041 %	0,1767 %	0,5505 %

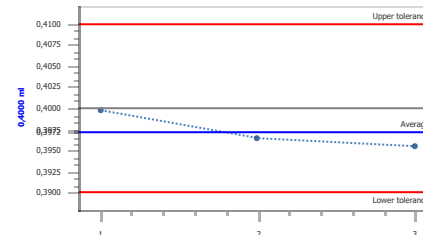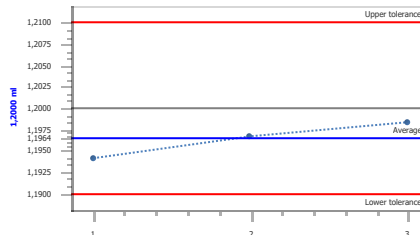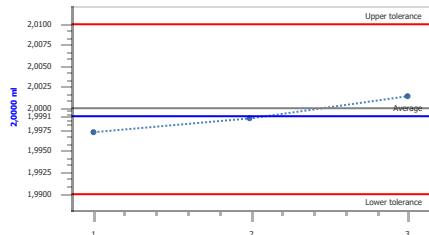

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

08.07.2026

Balance:

Sartorius -
LE244S-OCE

DE-M