

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 010 USP

**Graduated cylinders, 100:1 ml, USP, A, conf. cert.**




**Batch:** 13-25

**Serial:**

**Measuring Nr.** 72491

**Batch size:** 500

|                        |                   |                   |                    |
|------------------------|-------------------|-------------------|--------------------|
| <b>Volume:</b>         | <b>20,0000 ml</b> | <b>60,0000 ml</b> | <b>100,0000 ml</b> |
| <b>Tolerance:</b>      | $\pm 0,5000$ ml   | $\pm 0,5000$ ml   | $\pm 0,5000$ ml    |
| <b>Average value:</b>  | 20,0452 ml        | 60,1210 ml        | 100,1250 ml        |
| <b>Deviation:</b>      | 0,0833 ml         | 0,0786 ml         | 0,0861 ml          |
| <b>Precision (CV):</b> | 0,4164 %          | 0,1310 %          | 0,0861 %           |

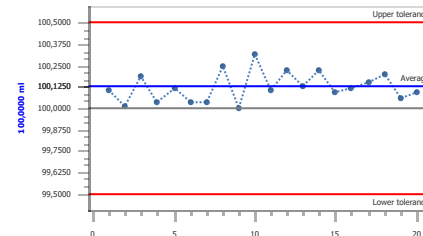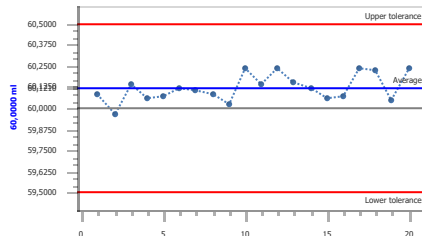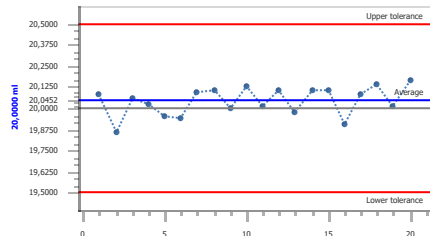

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:**

7

**Date:**

03.04.2025

**Balance:**

Sartorius -  
LE244S-OCE

DE-M