

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 100

Graduated cylinder, 1000:10 ml, A, conf. cert.




Batch: 26-25

Serial:

Measuring Nr. 73492

Batch size: 500

Volume:	200,0000 ml	600,0000 ml	1000,0000 ml
Tolerance:	$\pm 5,0000$ ml	$\pm 5,0000$ ml	$\pm 5,0000$ ml
Average value:	199,8709 ml	600,2368 ml	1000,3245 ml
Deviation:	0,6754 ml	0,9430 ml	1,2657 ml
Precision (CV):	0,3377 %	0,1572 %	0,1266 %

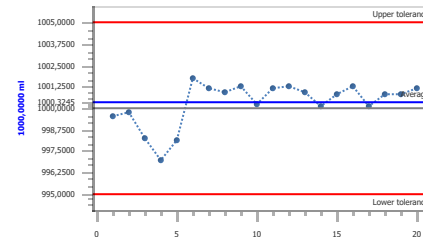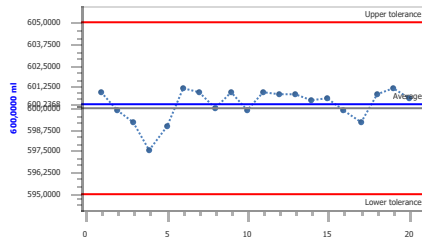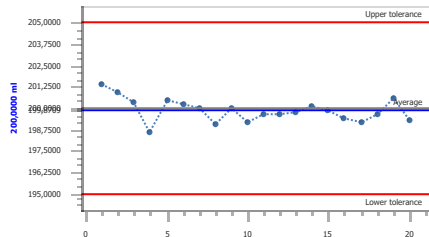

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

02.07.2025

Balance:

Sartorius -
MSE14202S-
OCE-D0

DE-M