

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 012 BL USP

Vol. flask, 10 ml, NS 10, blue grad., USP, A, conf. cert.

Batch: 29-25

Serial:

Measuring Nr. 73662

Batch size: 500


Volume: 10,0000 ml

Tolerance: $\pm 0,0200$ ml

Average value: 9,9995 ml

Deviation: 0,0022 ml

Precision (CV): 0,0215 %

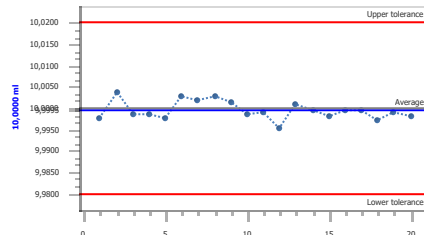

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

21.07.2025

Balance:

Sartorius -
LE244S-OCE

DE-M