

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 040

Volumetric flask, 400 ml, NS 19, A, KB

Batch: 16-25


Serial:

Measuring Nr. 72787

Batch size:

89

Volume:	400,0000 ml
Tolerance:	$\pm 0,2500$ ml
Average value:	400,0304 ml
Deviation:	0,0238 ml
Precision (CV):	0,0060 %

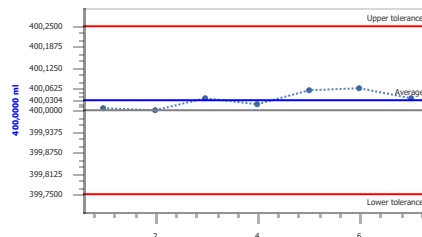

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

22.04.2025

Balance:

Sartorius - LA
1200 S

DE-M