

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 002 USP

Vol.flask, 20 ml, USP, NS 10, amber glass, A, conf.cert

Batch: 18-25


Serial:

Measuring Nr. 72901

Batch size:

268

Volume:	20,0000 ml
Tolerance:	$\pm 0,0300$ ml
Average value:	19,9981 ml
Deviation:	0,0057 ml
Precision (CV):	0,0283 %

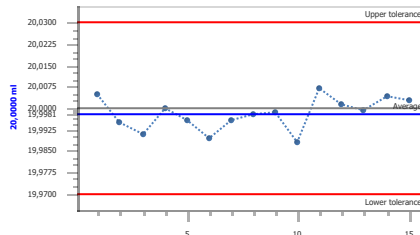

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

08.05.2025

Balance:

Sartorius -
LE244S-OCE

DE-M