

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 101 BL

Grad. pipettes, 1:0,01 ml, blue grad., AS, conf. cert.




Batch: 23-25

Serial:

Measuring Nr. 73642

Batch size: 150

Volume:	1,0000 ml	0,6000 ml	0,2000 ml
Tolerance:	$\pm 0,0070$ ml	$\pm 0,0070$ ml	$\pm 0,0070$ ml
Average value:	0,9998 ml	0,6029 ml	0,2017 ml
Deviation:	0,0026 ml	0,0016 ml	0,0008 ml
Precision (CV):	0,2556 %	0,2629 %	0,3859 %

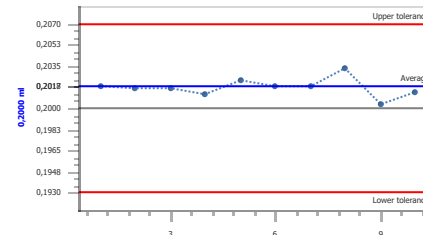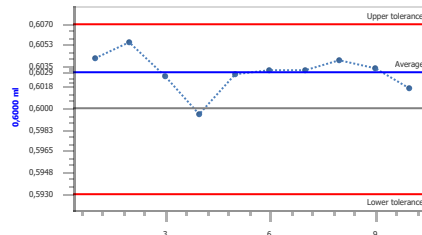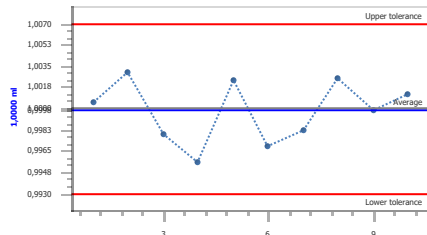

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

14.07.2025

Balance:

Sartorius -
LE244S-OCE

DE-M