

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 110

Grad. pipettes, 1:0,1 ml, AS, conf. cert.




Batch: 25-26

Serial:

Measuring Nr. 79397

Batch size: 280

Volume:	1,0000 ml	0,6000 ml	0,2000 ml
Tolerance:	$\pm 0,0070$ ml	$\pm 0,0070$ ml	$\pm 0,0070$ ml
Average value:	0,9977 ml	0,6011 ml	0,2006 ml
Deviation:	0,0018 ml	0,0019 ml	0,0012 ml
Precision (CV):	0,1767 %	0,3092 %	0,5833 %

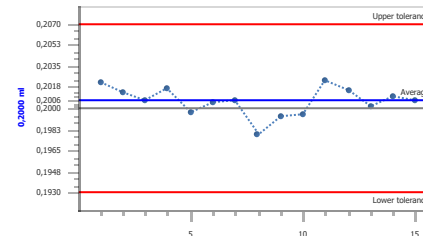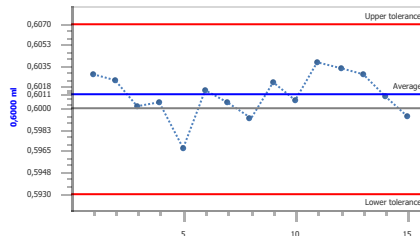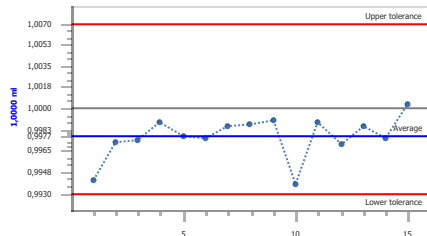

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

05.08.2026

Balance:

Sartorius -
LE244S-OCE

DE-M