

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 710

Graduated pipettes, 10:0,1 ml, AS, conf. cert.




Batch: 29-25

Serial:

Measuring Nr. 73923

Batch size: 3200

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	$\pm 0,0500$ ml	$\pm 0,0500$ ml	$\pm 0,0500$ ml
Average value:	10,0084 ml	5,9860 ml	1,9941 ml
Deviation:	0,0119 ml	0,0069 ml	0,0039 ml
Precision (CV):	0,1190 %	0,1158 %	0,1966 %

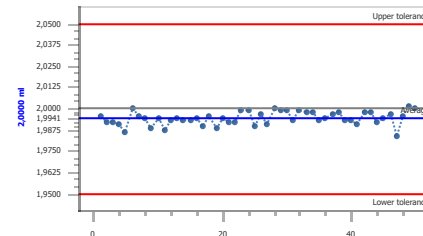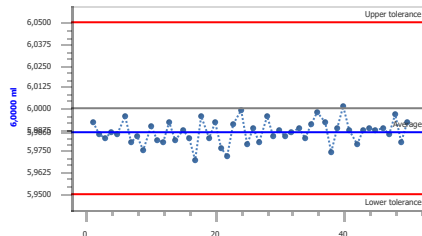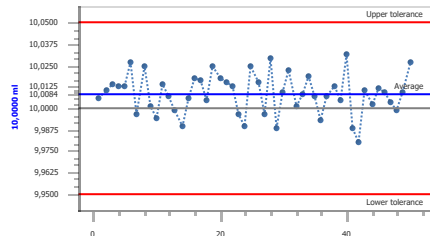

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

28.07.2025

Balance:

Sartorius -
LE244S-OCE

DE-M