

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 810

Graduated pipettes, 20:0,1 ml, AS, conf. cert.




Batch: 02-25

Serial:

Measuring Nr. 72181

Batch size: 1200

Volume:	20,0000 ml	12,0000 ml	4,0000 ml
Tolerance:	$\pm 0,1000$ ml	$\pm 0,1000$ ml	$\pm 0,1000$ ml
Average value:	19,9948 ml	12,0089 ml	4,0043 ml
Deviation:	0,0264 ml	0,0216 ml	0,0100 ml
Precision (CV):	0,1321 %	0,1800 %	0,2489 %

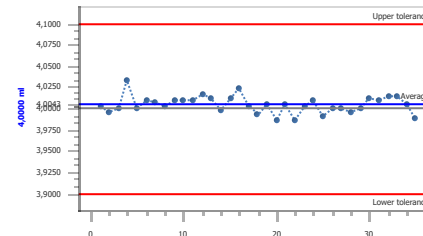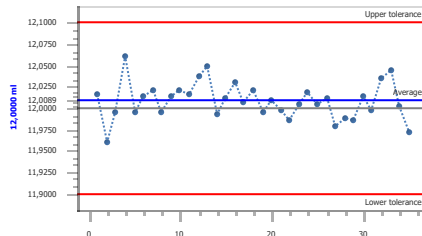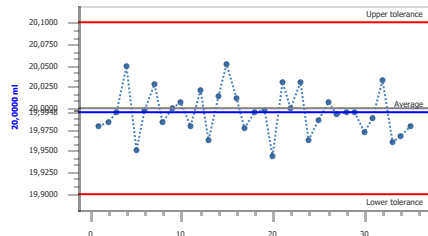

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

06.03.2025

Balance:

Sartorius -
LE244S-OCE

DE-M