

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 515 202

Graduated pipette, 2:0,02 ml, AS, conf. cert.




Batch: 28-25

Serial:

Measuring Nr. 73781

Batch size: 280

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	$\pm 0,0100$ ml	$\pm 0,0100$ ml	$\pm 0,0100$ ml
Average value:	2,0006 ml	1,2006 ml	0,4016 ml
Deviation:	0,0029 ml	0,0029 ml	0,0015 ml
Precision (CV):	0,1439 %	0,2422 %	0,3704 %

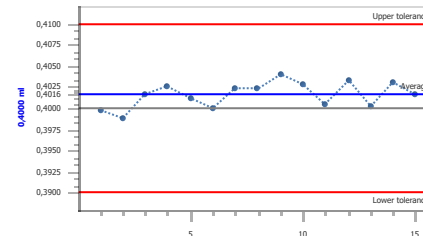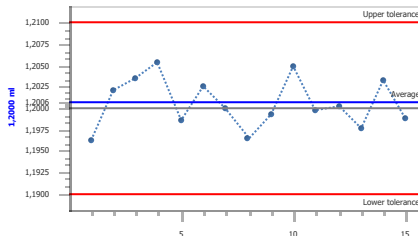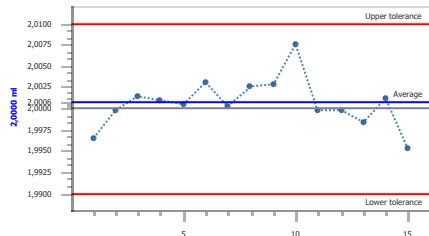

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

23.07.2025

Balance:

Sartorius -
LE244S-OCE

DE-M