

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 515 710

Grad. pipettes, 10:0,1 ml, AS, conf. cert.




Batch: 18-26

Serial:

Measuring Nr. 78800

Batch size: 1821

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	$\pm 0,0500$ ml	$\pm 0,0500$ ml	$\pm 0,0500$ ml
Average value:	9,9875 ml	5,9934 ml	2,0018 ml
Deviation:	0,0150 ml	0,0118 ml	0,0052 ml
Precision (CV):	0,1499 %	0,1971 %	0,2578 %

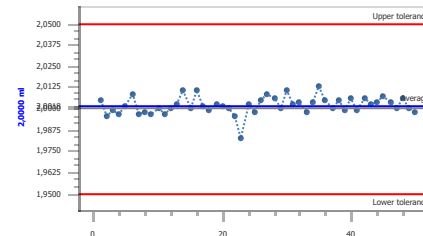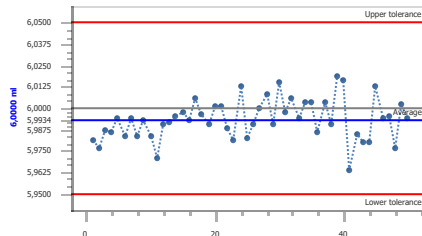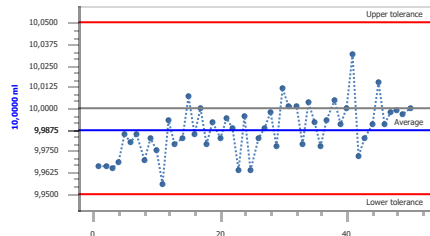

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

02.07.2026

Balance:

Sartorius -
LE244S-OCE

DE-M