

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 555 025

Volumetric pipettes, 2,5 ml, 2 marks, AS, conf. cert.

Batch: 14-25


Serial:

Measuring Nr. 73450

Batch size:

148

Volume:	2,5000 ml
Tolerance:	$\pm 0,0100$ ml
Average value:	2,5016 ml
Deviation:	0,0012 ml
Precision (CV):	0,0484 %

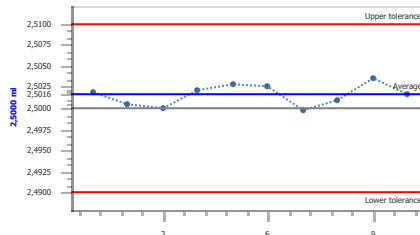

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

26.06.2025

Balance:

Sartorius -
LE244S-OCE

DE-M