

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 670 010

**Vol. flask, 100 ml, NS 12, amber glass, A, conf. cert.**

**Batch:** 13-25


**Serial:**

**Measuring Nr.** 72464

**Batch size:**

100

|                 |                 |
|-----------------|-----------------|
| Volume:         | 100,0000 ml     |
| Tolerance:      | $\pm 0,1000$ ml |
| Average value:  | 100,0120 ml     |
| Deviation:      | 0,0201 ml       |
| Precision (CV): | 0,0201 %        |

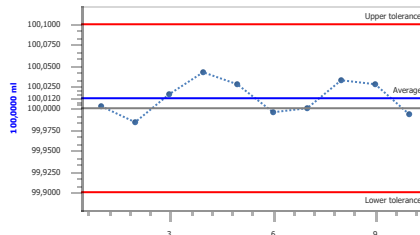

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:**

7

**Date:**

01.04.2025

**Balance:**

Sartorius -  
LE244S-OCE

DE-M