

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 010 053 B

Burettes, 5 ml, straight stopcock, AS, conf. cert.

Batch: 04-22




Serial:

Measuring Nr. 77759

Batch size:

27

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	$\pm 0,0100$ ml	$\pm 0,0100$ ml	$\pm 0,0100$ ml
Average value:	5,0029 ml	2,9991 ml	1,0014 ml
Deviation:	0,0032 ml	0,0034 ml	0,0009 ml
Precision (CV):	0,0636 %	0,1133 %	0,0918 %

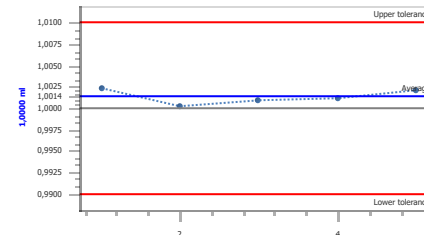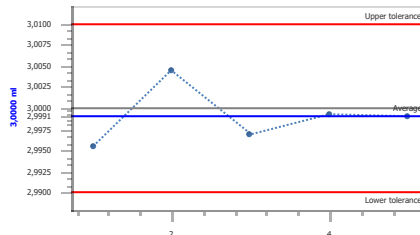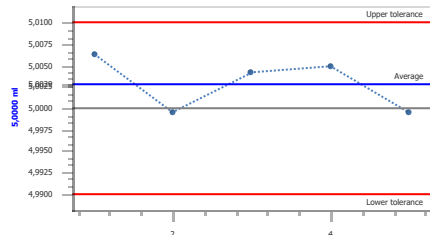

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

27.04.2026

Balance:

Sartorius -
LE244S-OCE

DE-M