

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 010 253

Burettes, 25 ml, str. stopcock, PTFE, AS, conf. cert.




Batch: 43-25

Serial:

Measuring Nr. 76599

Batch size: 50

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9975 ml	14,9951 ml	5,0016 ml
Deviation:	0,0065 ml	0,0044 ml	0,0045 ml
Precision (CV):	0,0261 %	0,0294 %	0,0898 %

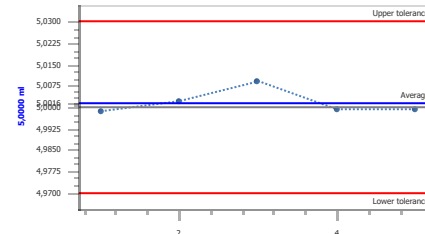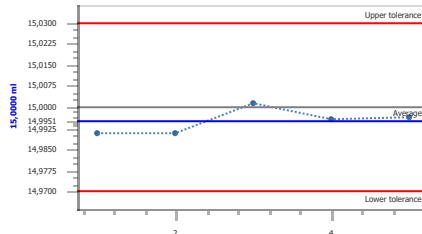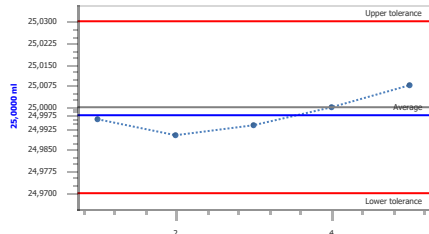

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	06.02.2026
Balance:	Sartorius - MSE224S-0CE -DU

