

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 012 053

**Burettes, 5 ml, str. stopc., PTFE- plug, AS, conf. cert.**




**Batch:** 40-25

**Serial:**

**Measuring Nr.** 75926

**Batch size:** 5

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	4,9978 ml	2,9950 ml	1,0001 ml
Deviation:	0,0037 ml	0,0021 ml	0,0026 ml
Precision (CV):	0,0747 %	0,0691 %	0,2551 %

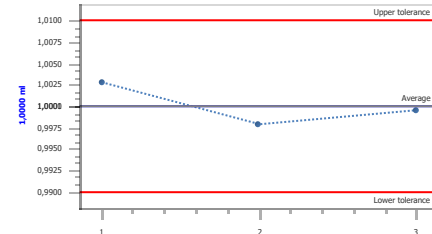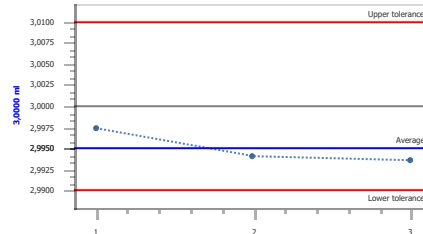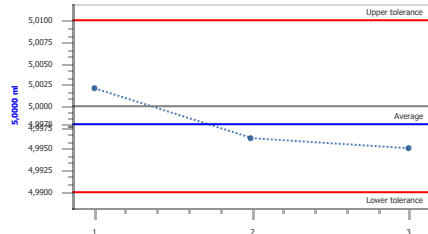

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	4
Date:	10.12.2025
Balance:	Sartorius - MSE224S-0CE -DU

