

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 012 102

**Burettes, 10 ml, str. stopcock, glass, AS, conf. cert.**




**Batch:** 43-20

**Serial:**

**Measuring Nr.:** 46191

**Batch size:** 10

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0047 ml	5,9991 ml	2,0007 ml
Deviation:	0,0073 ml	0,0019 ml	0,0026 ml
Precision (CV):	0,0735 %	0,0310 %	0,1311 %

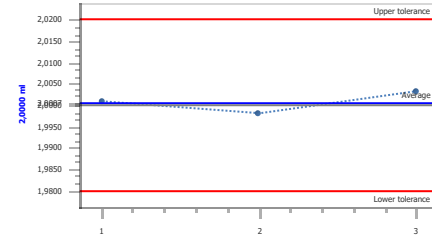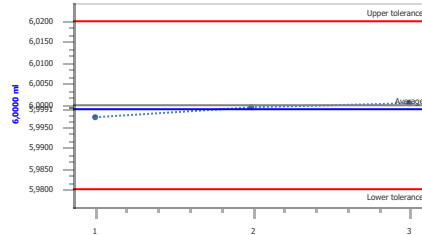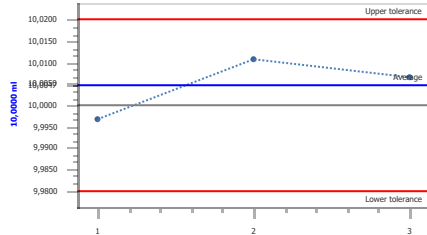

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	4
Date:	26.04.2021
Balance:	Sartorius - MSE224S-0CE -DU

