

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 104

Burettes, 10 ml, lateral stopcock, AS, conf. cert.

Batch: 43-19




Serial:

Measuring Nr.: 35160

Batch size:

2

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0088 ml	5,9998 ml	2,0005 ml
Deviation:	0,0055 ml	0,0027 ml	0,0037 ml
Precision (CV):	0,0554 %	0,0445 %	0,1873 %

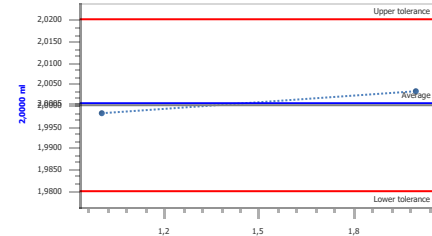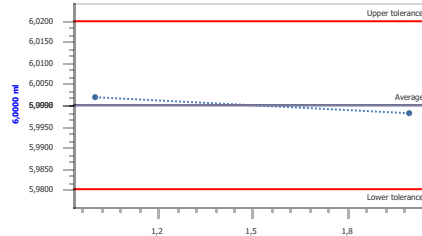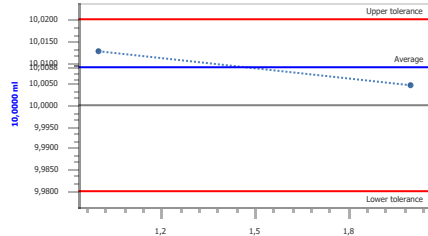

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

9

Date:

12.12.2019

Balance:

Sartorius -
LE244S-OCE

DE-M