

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 105

Burette, 10 ml, Schellb., lat. Valve, AS, conf. cert.




Batch: 45-25

Serial:

Measuring Nr. 76327

Batch size: 10

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0030 ml	5,9935 ml	2,0017 ml
Deviation:	0,0036 ml	0,0033 ml	0,0032 ml
Precision (CV):	0,0363 %	0,0546 %	0,1600 %

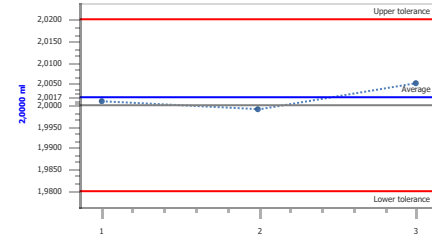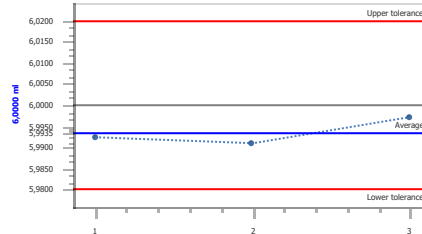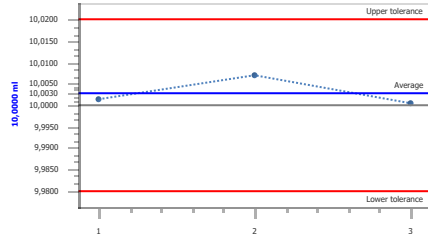

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	29.01.2026
Balance:	Sartorius - MSE224S-0CE -DU

