

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 253 TR

Burettes, 25 ml, with funnels, str. stopc., AS, conf. cert.




Batch: 38-15

Serial:

Measuring Nr. 19592

Batch size: 2

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9811 ml	14,9933 ml	4,9956 ml
Deviation:	0,0054 ml	0,0087 ml	0,0032 ml
Precision (CV):	0,0216 %	0,0577 %	0,0638 %

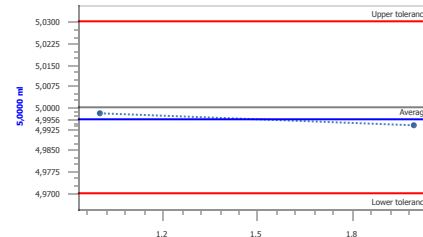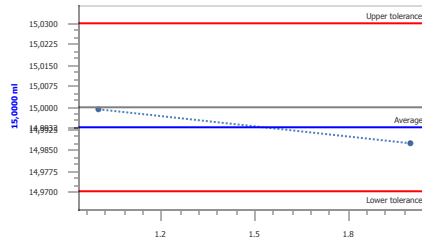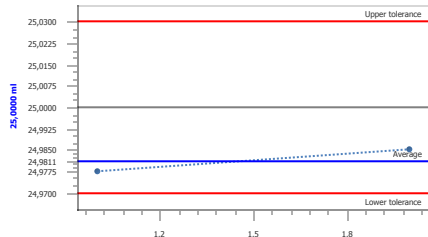

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	06.04.2018
Balance:	Sartorius - LE244S-OCE

DE-M