

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 255

Burettes, 25 ml, lat. needle valve, AS, conf. cert.




Batch: 43-25

Serial:

Measuring Nr. 76551

Batch size: 30

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9968 ml	14,9868 ml	4,9838 ml
Deviation:	0,0015 ml	0,0053 ml	0,0029 ml
Precision (CV):	0,0059 %	0,0354 %	0,0573 %

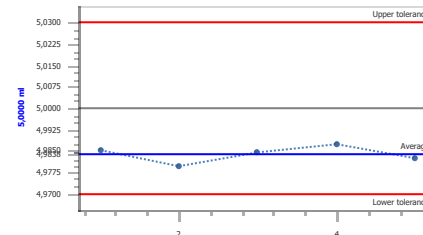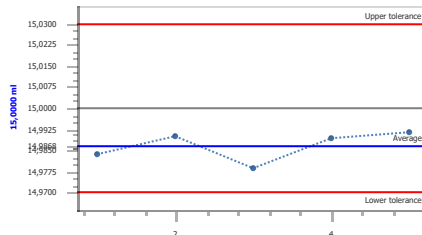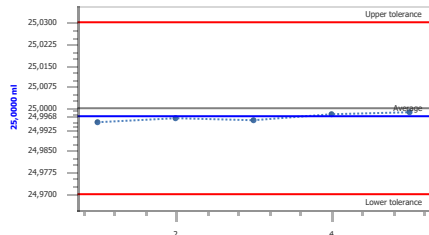

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	04.02.2026
Balance:	Sartorius - MSE224S-0CE -DU

DE-M