

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 502

Burettes, 50 ml, str. stopc., glass-plug, AS, conf. cert




Batch: 29-21

Serial:

Measuring Nr. 49347

Batch size: 30

Volume:	50,000 ml	30,000 ml	10,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0022 ml	30,0182 ml	10,0143 ml
Deviation:	0,0125 ml	0,0132 ml	0,0146 ml
Precision (CV):	0,0250 %	0,0440 %	0,1463 %

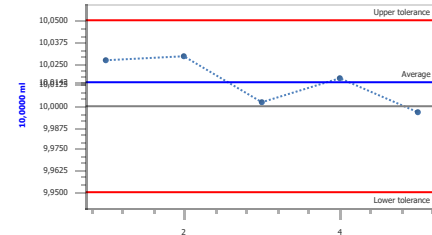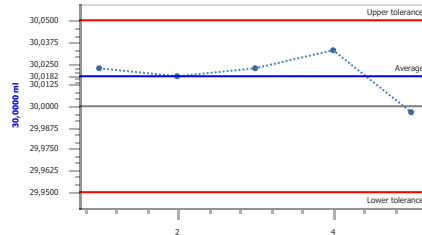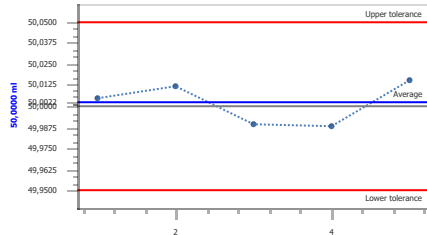

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	28.09.2021
Balance:	Sartorius - LE244S-OCE

