

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 503

Burettes, 50 ml, str. stopc., PTFE plug, AS, conf. cert.




Batch: 01-26

Serial:

Measuring Nr. 77475

Batch size: 100

Volume:	50,000 ml	30,000 ml	10,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0136 ml	30,0019 ml	10,0028 ml
Deviation:	0,0122 ml	0,0082 ml	0,0138 ml
Precision (CV):	0,0245 %	0,0272 %	0,1377 %

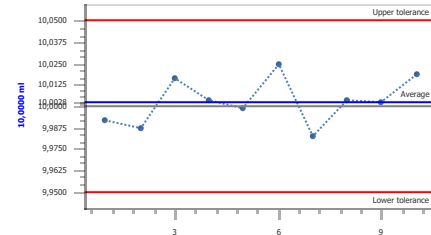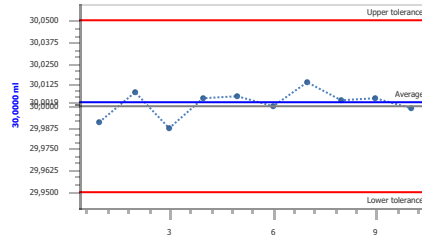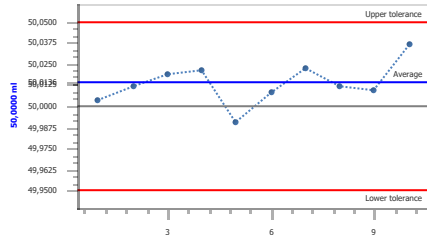

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	16.04.2026
Balance:	Sartorius - LE244S-OCE

