

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 504

Burettes, 50 ml, lat. stopc., Schellbach, AS, conf. cert.




Batch: 13-25

Serial:

Measuring Nr. 74436

Batch size: 15

Volume:	50,000 ml	30,000 ml	10,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0342 ml	30,0207 ml	10,0006 ml
Deviation:	0,0059 ml	0,0062 ml	0,0042 ml
Precision (CV):	0,0118 %	0,0206 %	0,0415 %

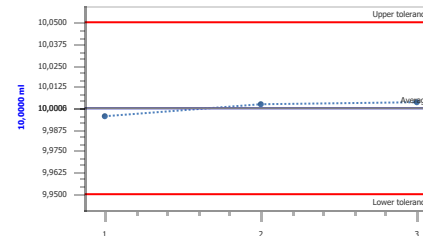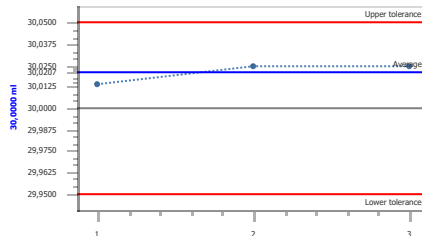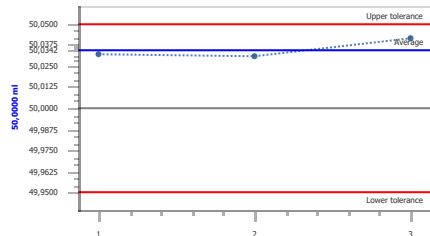

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	02.09.2025
Balance:	Sartorius - LE244S-OCE

DE-M