

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 903

Burettes, 100 ml, straight stopc., PTFE, AS, conf. cert.




Batch: 04-18

Serial:

Measuring Nr. 19039

Batch size: 30

Volume:	100,000 ml	60,000 ml	20,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	99,9553 ml	59,9984 ml	19,9778 ml
Deviation:	0,0056 ml	0,0241 ml	0,0202 ml
Precision (CV):	0,0056 %	0,0401 %	0,1011 %

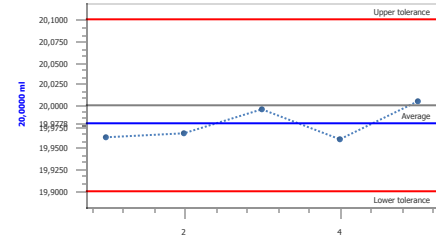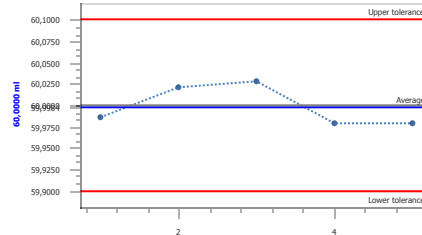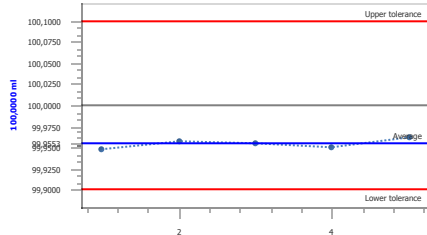

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	21.03.2018
Balance:	Sartorius - LE244S-OCE

DE-M