

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 052

Burettes, 5 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 36-16

Serial:

Measuring Nr. 23529

Batch size: 4

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	4,9995 ml	2,9939 ml	0,9963 ml
Deviation:	0,0036 ml	0,0007 ml	0,0011 ml
Precision (CV):	0,0720 %	0,0221 %	0,1058 %

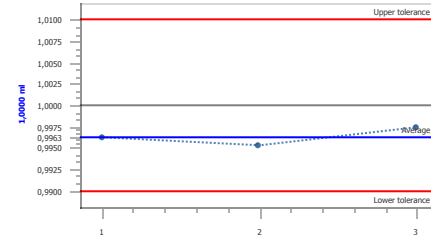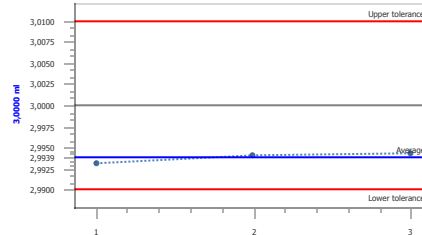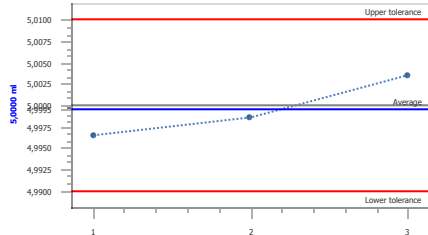

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	27.08.2018
Balance:	Sartorius - LE244S-OCE

