

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 103

Burettes, 10 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 43-19

Serial:

Measuring Nr. 34630

Batch size: 90

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	9,9973 ml	5,9956 ml	2,0014 ml
Deviation:	0,0033 ml	0,0047 ml	0,0027 ml
Precision (CV):	0,0328 %	0,0791 %	0,1359 %

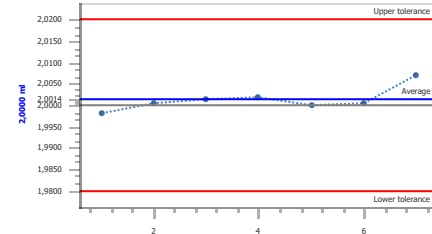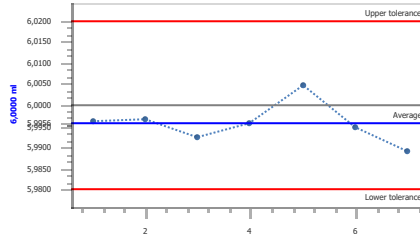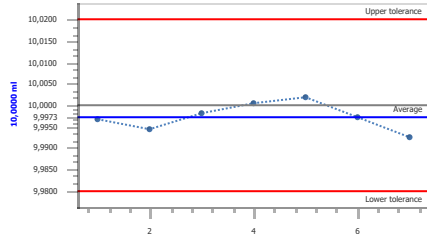

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	22.11.2019
Balance:	Sartorius - LE244S-OCE

