

# Certificate of performance



**Article:** 3 014 103

**Burettes, 10 ml, str. stopc., amber glass, AS, conf. cert.**




**Batch:** 29-21

**Serial:**

**Measuring Nr.** 54563

**Batch size:** 20

Volume:	10,000 ml	6,000 ml	2,000 ml
<b>Tolerance:</b>	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
<b>Average value:</b>	9,9928 ml	5,9934 ml	1,9983 ml
<b>Deviation:</b>	0,0051 ml	0,0039 ml	0,0040 ml
<b>Precision (CV):</b>	0,0506 %	0,0654 %	0,2009 %

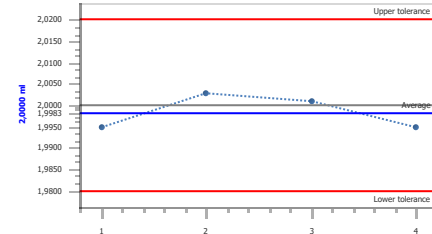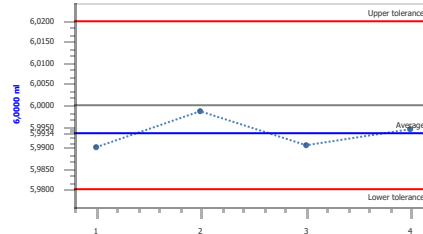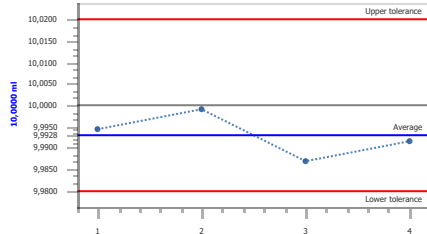

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	25.04.2022
<b>Balance:</b>	Sartorius - LE244S-OCE

