

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 103

Burettes, 10 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 11-22

Serial:

Measuring Nr. 56334

Batch size: 20

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	9,9941 ml	5,9912 ml	1,9999 ml
Deviation:	0,0061 ml	0,0042 ml	0,0046 ml
Precision (CV):	0,0611 %	0,0701 %	0,2299 %

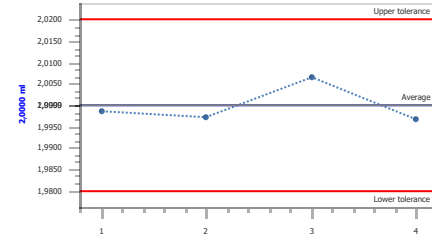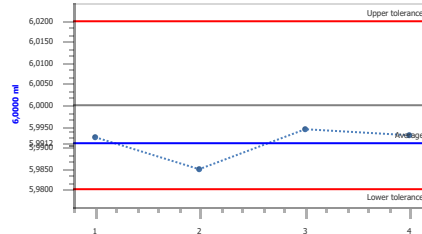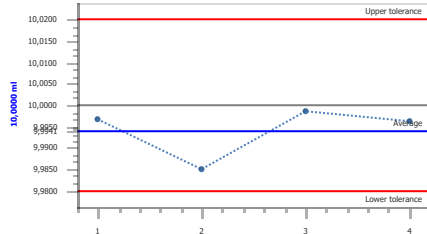

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	30.05.2022
Balance:	Sartorius - LE244S-OCE

