

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 104

Burettes, 10 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 05-20

Serial:

Measuring Nr.: 42739

Batch size: 3

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	9,9961 ml	5,9930 ml	1,9986 ml
Deviation:	0,0061 ml	0,0051 ml	0,0014 ml
Precision (CV):	0,0607 %	0,0854 %	0,0687 %

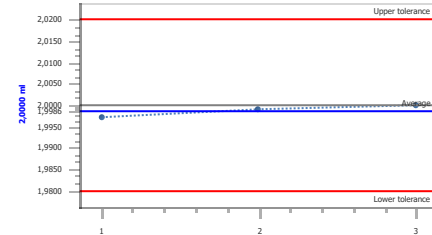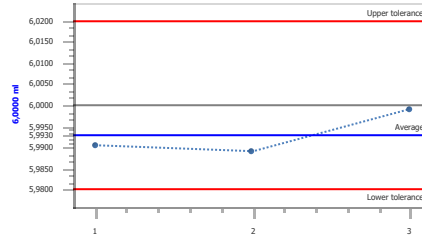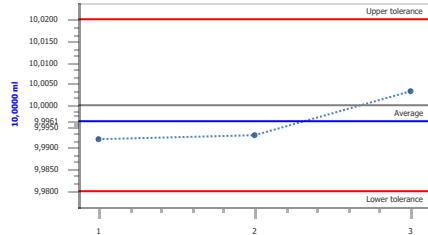

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	23.11.2020
Balance:	Sartorius - MSE224S-0CE -DU

DE-M