

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 253

Burettes, 25 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 05-23

Serial:

Measuring Nr. 63597

Batch size: 50

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0118 ml	15,0015 ml	5,0062 ml
Deviation:	0,0075 ml	0,0111 ml	0,0045 ml
Precision (CV):	0,0300 %	0,0740 %	0,0908 %

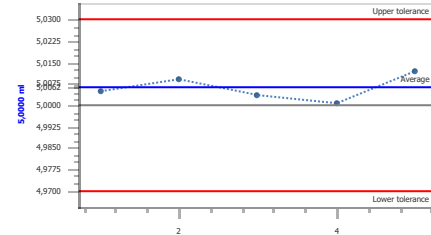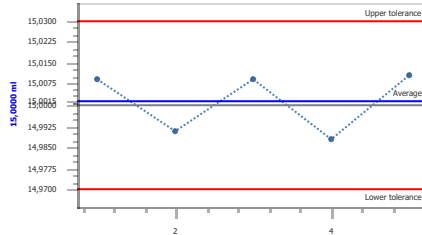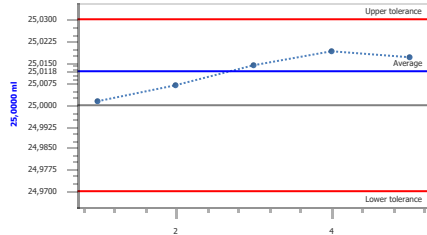

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	05.07.2023
Balance:	Sartorius - LE244S-OCE

