

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 503

Burettes, 50 ml, str. stopc., amber glass, AS, conf. cert.

Batch: 46-25




Serial:

Measuring Nr. 77928

Batch size:

50

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	49,9882 ml	29,9834 ml	9,9840 ml
Deviation:	0,0119 ml	0,0119 ml	0,0069 ml
Precision (CV):	0,0238 %	0,0397 %	0,0693 %

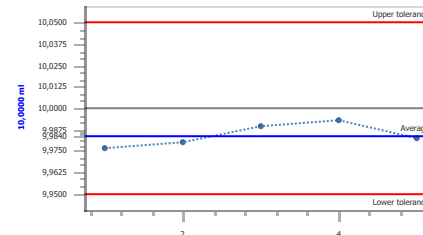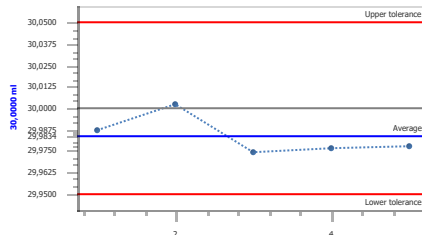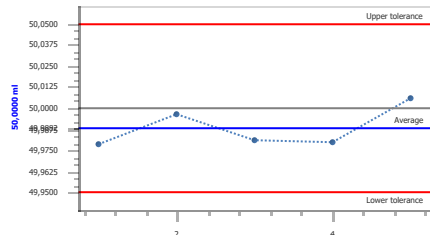

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

30.04.2026

Balance:

Sartorius -
LE244S-OCE

DE-M