Certificate of performance


witeg GERMANY

ISO 9001 CERTIFIED

Article:	**3 014 503**
Burettes, 50 ml, str. stopc., amber glass, AS, conf. cert.	

Batch:	46-25	**Serial:**	
Measuring Nr.	80456	**Batch size:**	49

Volume:	**50,0000 ml**	**30,0000 ml**	**10,0000 ml**
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0170 ml	29,9856 ml	9,9928 ml
Deviation:	0,0147 ml	0,0144 ml	0,0076 ml
Precision (CV):	0,0294 %	0,0479 %	0,0763 %

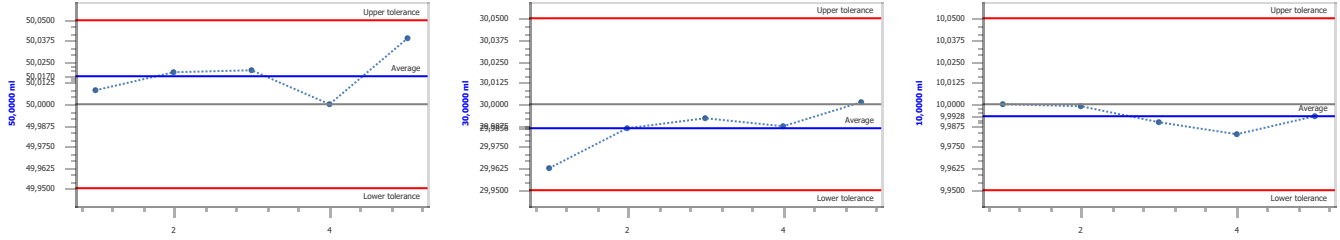

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH
Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	30.10.2026
Balance:	Sartorius - LE244S-0CE

DE-M