

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 022 057

**Burette, 5 ml, straight needle valve, AS, conf. cert.**




**Batch:** 12-23

**Serial:**

**Measuring Nr.:** 62388

**Batch size:** 10

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	4,9995 ml	2,9921 ml	1,0015 ml
Deviation:	0,0033 ml	0,0009 ml	0,0027 ml
Precision (CV):	0,0652 %	0,0305 %	0,2662 %

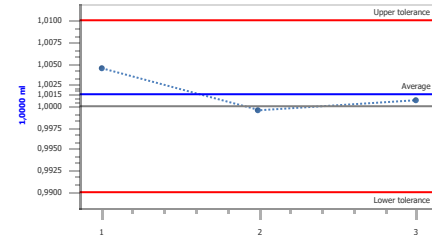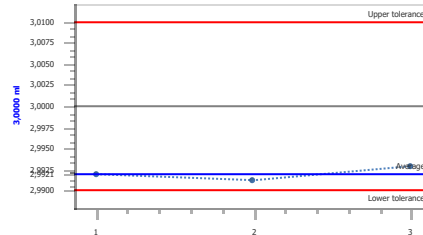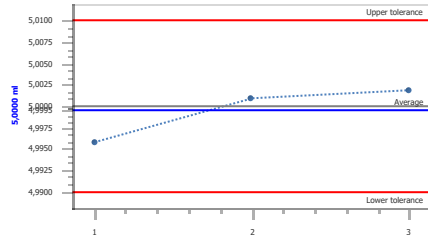

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	31.03.2023
Balance:	Sartorius - LE244S-OCE

