

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 022 107

Burettes, 10 ml, str. needle valve, AS, conf. cert.




Batch: 32-18

Serial:

Measuring Nr. 27529

Batch size: 2

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0108 ml	6,0020 ml	2,0010 ml
Deviation:	0,0041 ml	0,0051 ml	0,0018 ml
Precision (CV):	0,0412 %	0,0852 %	0,0887 %

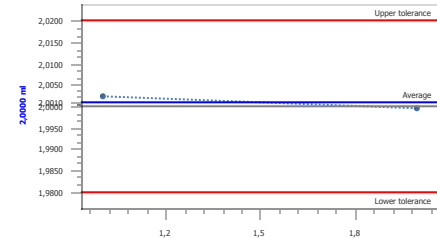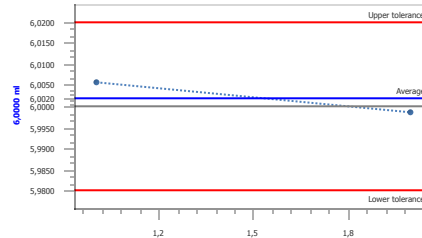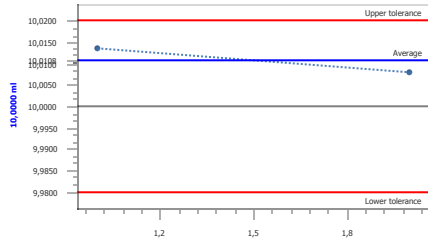

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	06.02.2019
Balance:	Sartorius - LE244S-OCE

DE-M