

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 022 507

Burettes, 50 ml, straight needle valve, AS, conf. cert.




Batch: 25-20

Serial:

Measuring Nr. 39990

Batch size: 13

Volume:	50,000 ml	30,000 ml	10,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	49,9876 ml	29,9990 ml	10,0202 ml
Deviation:	0,0114 ml	0,0062 ml	0,0058 ml
Precision (CV):	0,0229 %	0,0207 %	0,0583 %

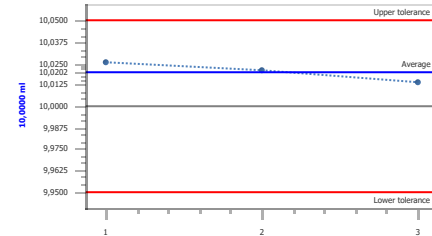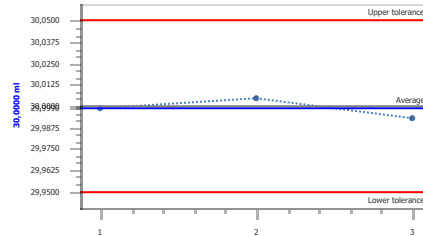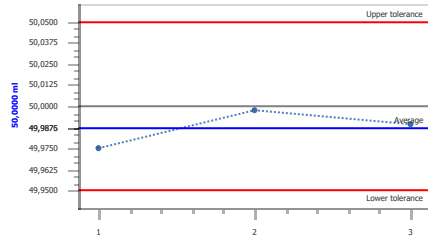

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	08.09.2020
Balance:	Sartorius - LE244S-OCE

DE-M