

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 105

Pellet-burettes, 10 ml, lat. needle valve, AS, conf. cert.




Batch: 09-21

Serial:

Measuring Nr.: 51581

Batch size: 10

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	9,9958 ml	5,9945 ml	2,0044 ml
Deviation:	0,0033 ml	0,0036 ml	0,0035 ml
Precision (CV):	0,0328 %	0,0607 %	0,1728 %

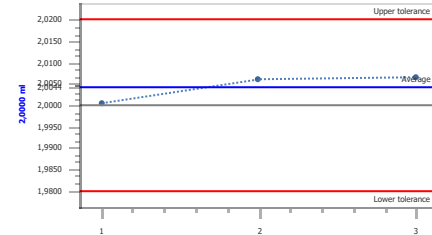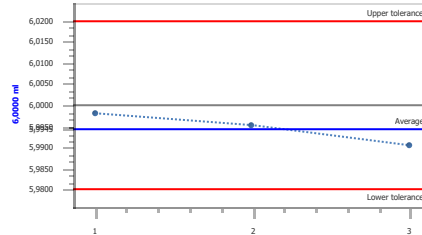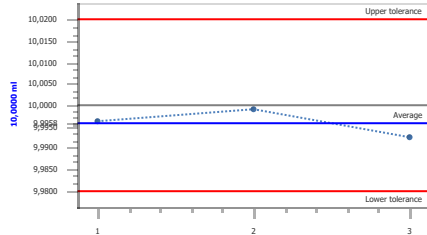

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	26.01.2022
Balance:	Sartorius - LE244S-0CE

