

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 122 255

**Pellet-burettes, 25 ml, lat. needle valve, AS, conf. cert.**




**Batch:** 07-20

**Serial:**

**Measuring Nr.:** 42359

**Batch size:** 10

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9911 ml	14,9938 ml	5,0058 ml
Deviation:	0,0086 ml	0,0111 ml	0,0063 ml
Precision (CV):	0,0345 %	0,0740 %	0,1255 %

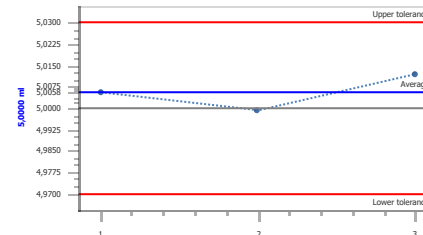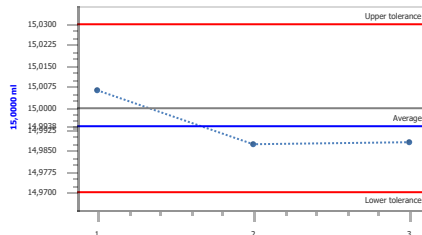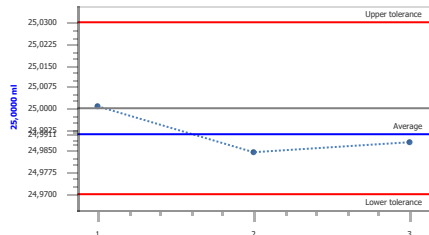

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	4
Date:	10.11.2020
Balance:	Sartorius - MSE224S-0CE -DU

