

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 255

Pellet-burettes, 25 ml, lat. needle valve, AS, conf. cert.




Batch: 29-20

Serial:

Measuring Nr.: 43438

Batch size: 12

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0063 ml	15,0097 ml	5,0194 ml
Deviation:	0,0105 ml	0,0060 ml	0,0024 ml
Precision (CV):	0,0418 %	0,0397 %	0,0471 %

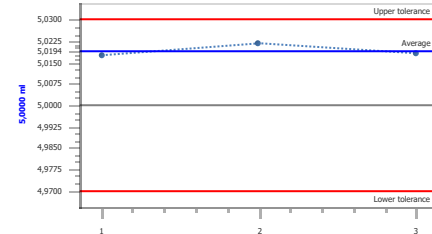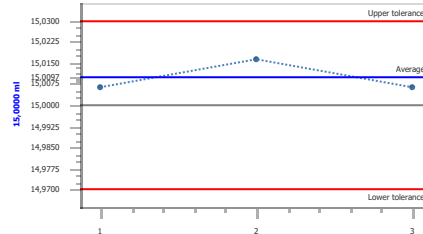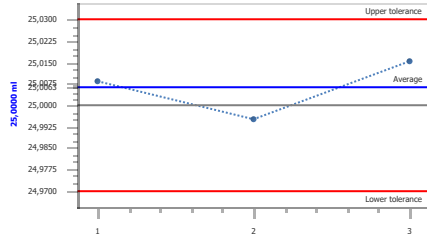

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	05.01.2021
Balance:	Sartorius - MSE224S-0CE -DU

