

Certificate of performance



Article: 3 122 255

Pellet-burettes, 25 ml, lat. needle valve, AS, conf. cert.




Batch: 11-22

Serial:

Measuring Nr.: 59646

Batch size: 20

| Volume: | 25,0000 ml | 15,0000 ml | 5,0000 ml |
|-----------------|-------------|-------------|-------------|
| Tolerance: | ± 0,0300 ml | ± 0,0300 ml | ± 0,0300 ml |
| Average value: | 24,9982 ml | 14,9962 ml | 5,0121 ml |
| Deviation: | 0,0096 ml | 0,0052 ml | 0,0061 ml |
| Precision (CV): | 0,0386 % | 0,0347 % | 0,1217 % |

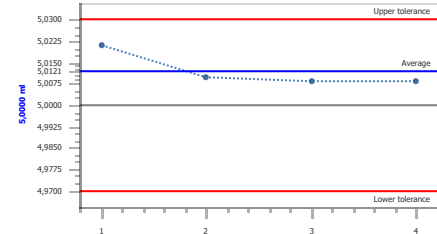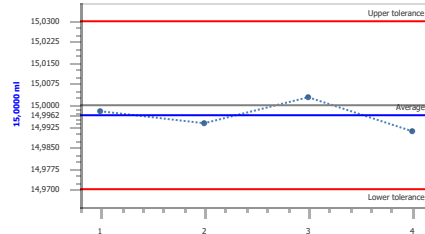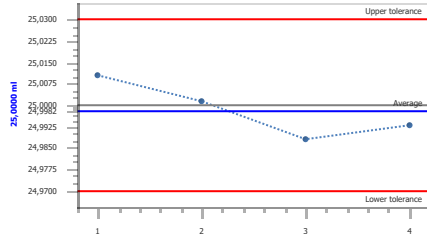

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|-----------|-----------------------------------|
| Operator: | 4 |
| Date: | 11.10.2022 |
| Balance: | Sartorius - MSE224S-0CE -DU |

