

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 122 258

**Pellet-burettes, 25 ml, lat. needle valve, AS, conf. cert.**




**Batch:** 11-24

**Serial:**

**Measuring Nr.** 71400

**Batch size:** 20

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0116 ml	15,0059 ml	5,0046 ml
Deviation:	0,0048 ml	0,0059 ml	0,0089 ml
Precision (CV):	0,0190 %	0,0396 %	0,1775 %

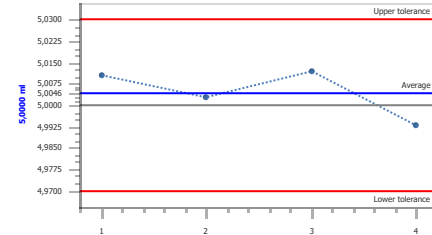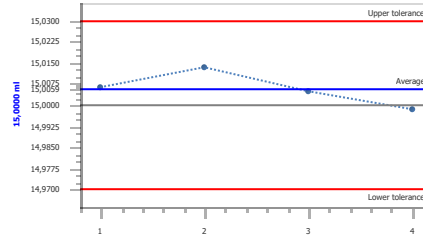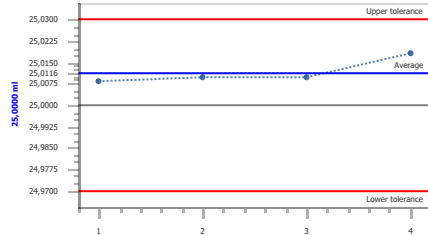

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	21.01.2025
Balance:	Sartorius - LE244S-OCE

