

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 505

Pellet-burettes, 50 ml, lat. needle valve, AS, conf. cert.




Batch: 13-19

Serial:

Measuring Nr. 31031

Batch size: 30

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0128 ml	30,0268 ml	10,0339 ml
Deviation:	0,0180 ml	0,0100 ml	0,0078 ml
Precision (CV):	0,0359 %	0,0334 %	0,0782 %

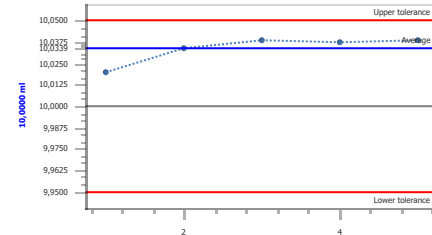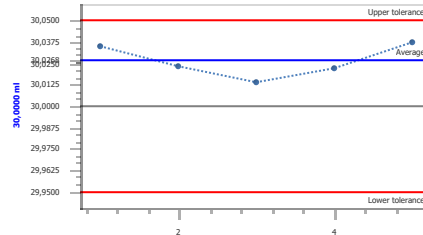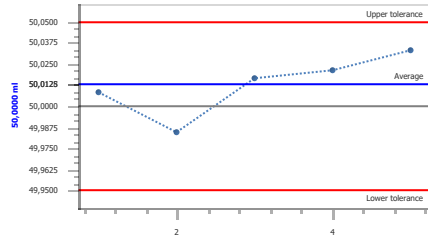

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	04.07.2019
Balance:	Sartorius - LE244S-OCE

